Switch off Evita 4 / Evita 2 / EvitaXL dura and unplug from mains.

Remove CO2-carrier PCB from device by unscrewing both fixing screws on right and left in the fixing bracket.

Ensure that the jumpers on processor board PCB 68 70 133 and signal processor PCB 68 70 296 are connected correctly (see drawing page 4).

Using distance bolts 83 05 182, sealing rings D 4766 and screws 13 30 799, attach the two PCBs of the CO2-module 68 70 132 (83 50 411) and 68 70 133 (68 70 296) to the CO2-carrier PCB as shown in the drawing.

Insert cable harness 83 06 567 and 83 06 766 as shown in the drawing (page 3). The groove of the plug should point upwards.

Insert CO2-carrier PCB and screw fixing screws back in.

Evita 4:
Start up Evita 4 and change to configuration menu. Press ”System Defaults” softkey and then ”Service”. A numeric keyboard appears. Enter the code ”6795”.

Evita 2 dura:
Start up Evita 2 dura and change to configuration menu with the softkey ”Calib./Config”
Press ”Ventilation” softkey. A numeric keyboard appears. Enter the code ”6795”with the rotary knob.

Wait at least 15 seconds. Then switch off device.

Switch device back on and perform zero calibration and filter test as described in the Instruction for Use.

For both devices perform test for electrical safety (patient leakage current) and functional test.

EvitaXL:
Start up EvitaXL and press the "System/Setup" hardkey. Click on the "Service" tab, and a numerical keypad appears. Enter the code "6795". "OK" will appear in the field next to the word "Code".

Schutz nach DIN 34 beansprucht.
Use of this document / contents is forbidden without express authority. All rights reserved.
Dräger Medical AG & Co. KGaA, D-23542 Lübeck

Schutz nach DIN 34 beansprucht.
Use of this document / contents is forbidden
without express authority. All rights reserved.
Dräger Medical AG & Co. KGaA, D-23542
Lübeck

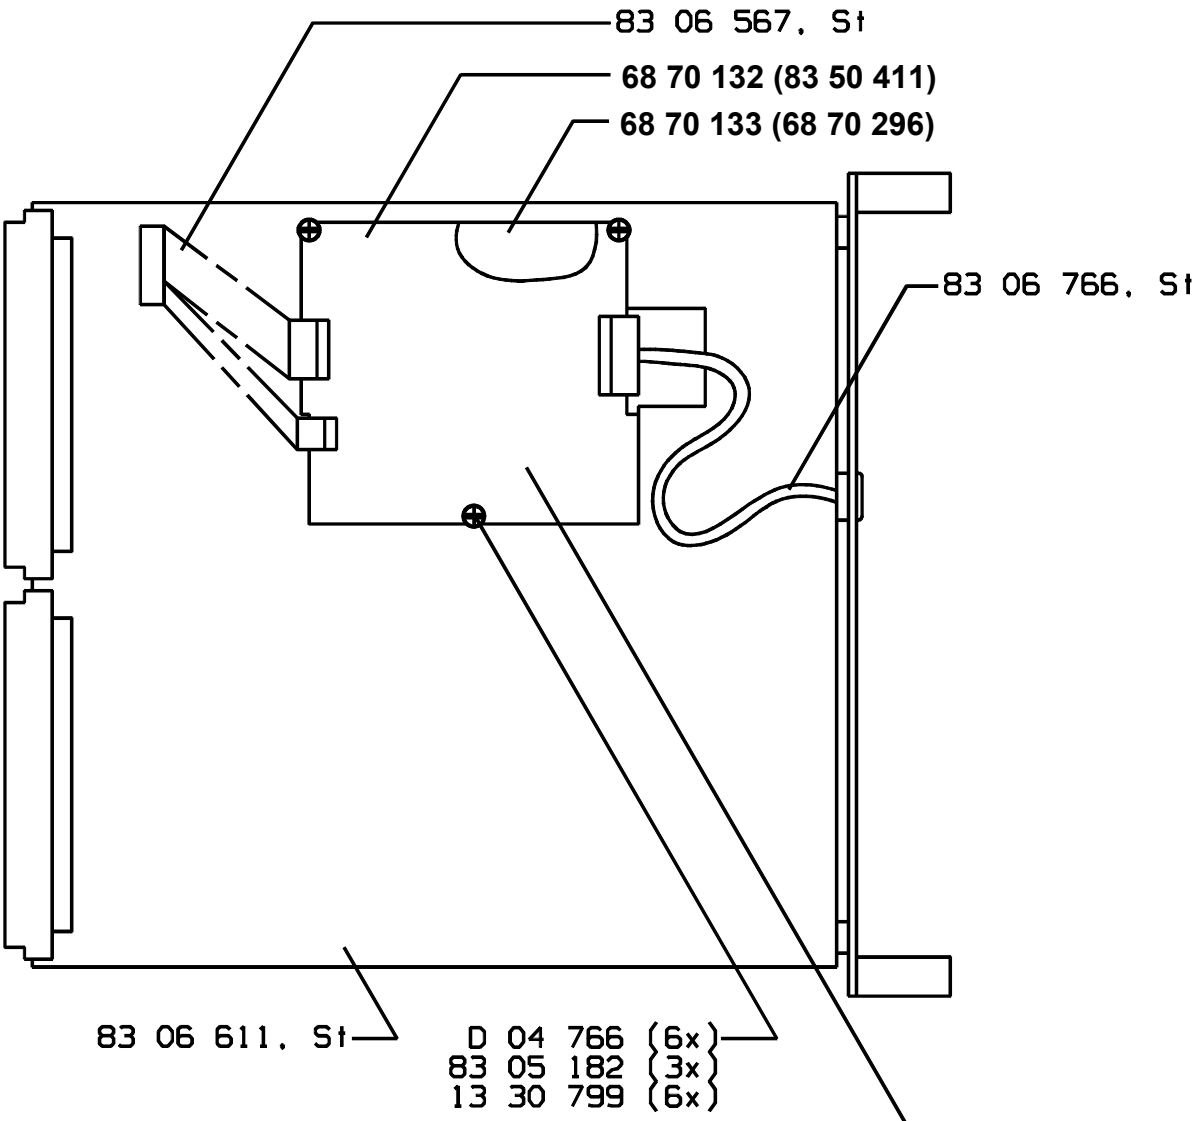

Modul mounted on side A
Processor Board
(signal processor PCB) below

Schutz nach DIN 34 beansprucht.
Use of this document / contents is forbidden
without express authority. All rights reserved.
Dräger Medical AG & Co. KGaA, D-23542
Lübeck

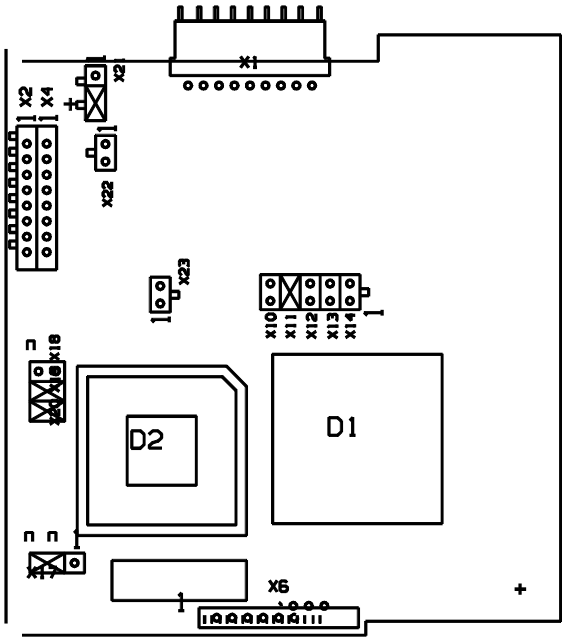

X10 open
X11 closed
X12 open
X13 open
X14 open
X17 on 2 and 3 closed

X18 open
X19 closed
X20 closed
X21 on 2 and 3 closed
X22 open
X23 open